Date: October 20, 2015

MALABAR

INTERNATIONAL

AIRCRAFT MAINTENANCE & SUPPORT EQUIPMENT

OWNER'S MANUAL FOR MALABAR MODEL

PF54115-58

2 GALLON FLUID DISPENSER



THIS INSTRUCTION MANUAL * GENERAL DESCRIPTION

- * OPERATION
- * SERVICE
- * PARTS BREAKDOWN

For Service & Spare Parts, Please Contact:

Malabar International 220 W. Los Angeles Avenue Simi Valley, California 93065 Phone: (805) 581-0116 Fax: (805) 584-1624 E-mail: sales@malabar.com Web site: http://www.malabar.com

OVER 65 YEARS OF SERVICE & EXPERIENCE

© 2002 Malabar International. All rights reserved. Permission to reproduce all or part of this material must be obtained from Malabar International.

GENERAL DESCRIPTION, OPERATION, SERVICE AND PARTS BREAKDOWN

MALABAR MODEL PF54115-58 2 GALLON FLUID DISPENSER

CAUTION: AIRCRAFT MANUFACTURER'S SPECIFICATIONS AND INSTRUCTIONS MUST BE FOLLOWED. IN THE EVENT OF CONTRADICTION BETWEEN AIRCRAFT MANUFACTURER'S SPECIFICATIONS AND MALABAR'S, AIRCRAFT MANUFACTURER'S WILL PREVAIL.

SPECIFICATIONS:

Fluid	SKYDROL LD4	
Reservoir capacity	2 U.S. gal	7.6 liters
Pump outlet pressure	100 psig	689 kPa
Volume per stroke	2.5 cubic in	41 cc
Hose length	120 in	3048 mm
Net weight (empty)	12 lbs	5.4 kg
Filter rating	3 micron nominal	
Fluid tank	stainless steel	

GENERAL DESCRIPTION:

The Malabar Model PF54115-58 is a 2 gallon fluid dispenser used to service various commercial aircraft. The hand pump dispenser consists of a reservoir, pump assembly, filter assembly, fillport assembly and a fluid delivery hose.

PREPARATION FOR USE:

The unit is shipped fully assembled. Fill reservoir at fillport with approved fluid. Operate hand pump assembly a few strokes to bleed all air out of the system. The unit is now ready for use.

OPERATION:

1. Connect the hose to the aircraft service.

2. Use full steady pumping strokes when operating pump assembly during replenishing.

3. Disconnect the hose from the aircraft service point and store the unit in a dry, dust free location.

ILLUSTRATED PARTS LIST:

Refer to figure 1A & 1B for unit assembly (see sheets 3 & 4) or figure 2 for pump assembly (see sheet 5).

SERVICING:

1. The frequency of filter change depends on operating conditions. Generally, changes should be made every 3-4 months or sooner if more than normal resistance is felt on the pumping stroke at low pressure. Refer to item 6 in figure 1A (see sheet 3) to change element.

REPAIR AND REPLACEMENT:

No definite time schedule can be established for the overhaul of the pump assembly for the replacement of the various moving parts. The number of times the pump assembly is operated materially affect the life of the working parts. The moving piston seal (item 4) and rod seal (item 14) are normally the first to wear (see sheet 5). This is usually indicated by leakage of fluid past the piston or rod. It is advisable to change piston seal (item 4), rod seal (item 14) and gasket (item 13) immediately if leakage is discovered. A repair parts kit (P/N PF2-68PK) is available and recommended to keep on hand at your facility. Refer to sheet 6 for the complete list of parts contained in the repair parts kit.

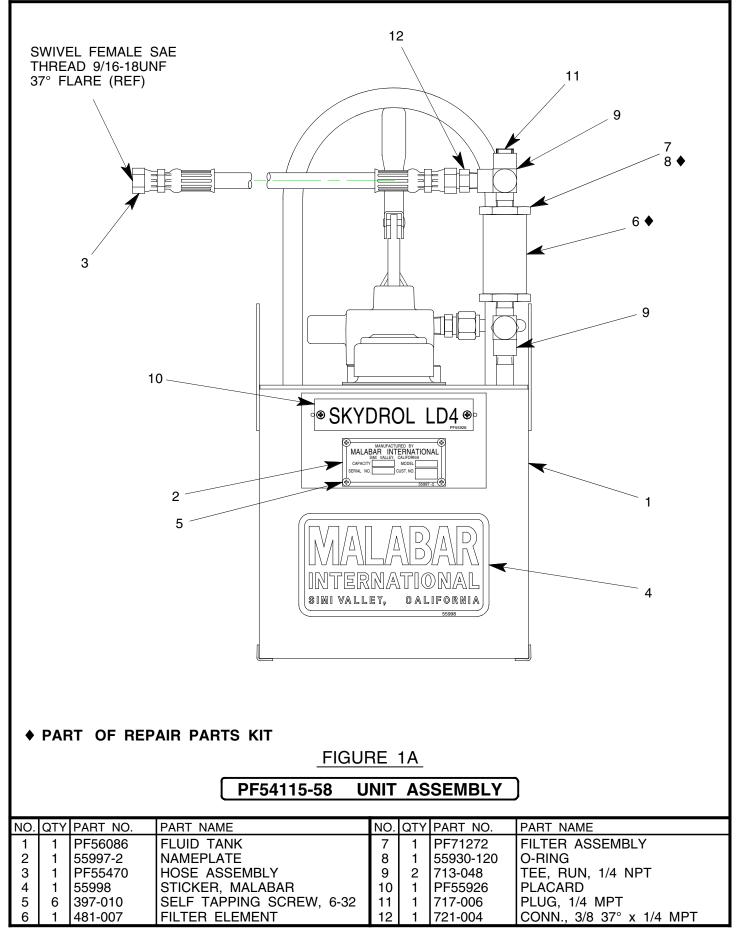


FIGURE 1B PF54115-58 UNIT ASSEMBLY NO. QTY PART NO. PART NAME NO. QTY PART NO. PART NAME
1 1 PF55447 FILLPORT ASSY 5 5 323-038 SHCS, 1/4-28 x 1 3/4 LG 2 1 PF53415A-2 PUMP ASSEMBLY 6 1 323-063 SHCS, 1/4-28 x 1" LG 3 1 PF55672 GASKET 7 1 732-010 TUBING, 3/8 OD x .065 WAL 4 2 721-009 CONN., 3/8 TUBE x 1/4 MPT - - - -

